

A new charged particle detector for the KOTO experiment at J-PARC

H M Kim for the KOTO Collaboration

Division of Science Education, Jeonbuk National University, Jeonju 54896, Republic of Korea

E-mail: recenter@naver.com

Abstract. We report the performance of a new scintillator array Downstream Charged Veto (DCV) for the J-PARC KOTO experiment to suppress the $K_L \rightarrow \pi^+\pi^-\pi^0$ decay background. Since the background originates from undetected charged pions passing through the beam hole of the electromagnetic calorimeter, the DCV detector was installed in vacuum downstream of the calorimeter. The DCV is composed of two plastic scintillator pipes read out by Multi Pixel Photon Counters through wavelength shifting fibers. The light yield was found to be 60 photoelectrons/0.8 MeV in a test bench when cosmic-rays pass through the center of the DCV. Energy calibration was performed using cosmic-rays after installation.

1. Introduction

The KOTO experiment at J-PARC aims to study the $K_L \rightarrow \pi^0\nu\bar{\nu}$ decay, which is one of the most sensitive probes to new physics beyond the standard model (SM). Its signature is a pair of photons from a π^0 decay without any additional activity in the hermetic detector system surrounding the decay region. To detect this highly suppressed decay, expected at 3×10^{-11} in the SM, it is important to reject background events related to other kaon decay modes. At the single event sensitivity of 1.30×10^{-9} achieved with 2015 data by KOTO, the number of $K_L \rightarrow \pi^+\pi^-\pi^0$ background events was estimated to be 0.05 [1], which corresponds to 2 events at the SM sensitivity. The decay becomes background when charged pions passing through the beam hole are undetected due to their interaction with non-active materials. A Monte Carlo simulation shows that most of π^+ and π^- particles disappear in three sections, as illustrated in Figure 1. One is the membrane which separates the 10^{-5} Pa decay region and the 0.1 Pa detector region. Another source is square pipes made of 0.5-mm-thick G10 plates placed inside the calorimeter and the collar counter CC04 separately, which prevents the membrane from drooping toward the beam axis. The last one is a beam pipe made of 10-mm-thick aluminum for extending the vacuum region downstream.

To suppress the $K_L \rightarrow \pi^+\pi^-\pi^0$ background, such charged pions should be detected before they interact with those non-active materials. In this respect, we decided to install a new charged particle detector, named Downstream Charged Veto DCV, inside the high vacuum region downstream of the electromagnetic calorimeter. To maximize the detector performance, the DCV should be placed as close as possible to the calorimeter. Since the DCV is able to support the membrane, we do not need the G10-pipe inside the CC04 anymore. The G10-pipe placed inside the calorimeter is still needed, though its length can be shortened.

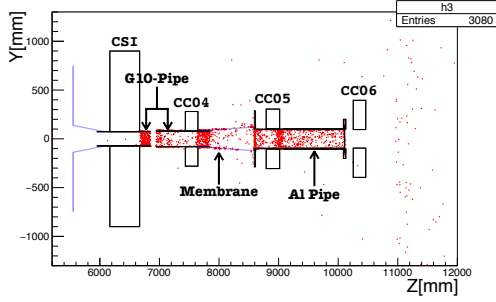


Figure 1. Interacting points of π^+ and π^- . Red dots indicate where the charged pions are disappeared.

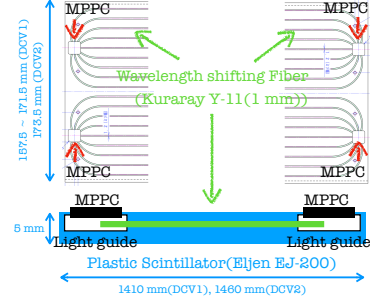


Figure 2. Configuration of scintillator with WLS fibers and MPPCs.

2. Structure of the DCV

The DCV consists of two successive square pipes, and each of them is made of 4 sheets of scintillators. The DCV1 is placed at 463 mm downstream from the calorimeter and inside the membrane, and the DCV2 is placed at 76 mm downstream from the DCV1 and inside the aluminum beam pipe. The DCV1 is a 1410-mm-long tapered square pipe with cross sections of 157.5 mm square at the upstream end and 171.5 mm square at the downstream end. The DCV2 is a 1460-mm-long square pipe with a side length of 173.5 mm. Wavelength shifting (WLS) fibers (Y11, Kuraray) with a diameter of 1 mm are embedded in 18 parallel grooves in a 5-mm-thick plastic scintillator (EJ-200, Eljen Technology). Due to the limited space for the DCV, we needed to attach the Multi Pixel Photon Counters (MPPCs) on the scintillator surface directly. An aluminum light guide for the MPPCs is placed in both ends of the scintillator, and the WLS fibers are routed into the light guide. Since the size of the light guide is $6 \times 6 \text{ mm}^2$ to fit the size of MPPC, the WLS fibers should be bent to converge into the light guide as shown in Figure 2. The curvature of grooves near the end of scintillator is designed to have a radius larger than 20 mm. The light loss increases rapidly below the radius of 20 mm, as illustrated in Figure 3. The WLS fibers are grouped into two and read by MPPC (S13360-6050PE, Hamamatsu) at both ends of each group (4 read-out MPPCs in total).

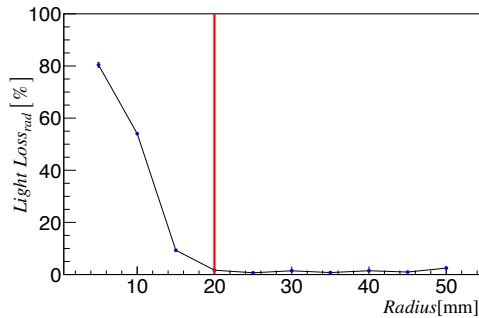


Figure 3. Light loss due to the curvature of the WLS fiber.

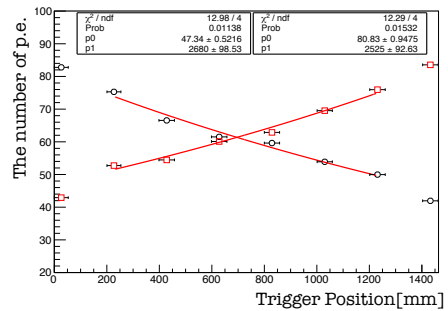


Figure 4. Number of photoelectrons at each cosmic-ray trigger point.

3. Fabrication Process

The WLS fibers were glued to the plastic scintillator plate using the optical cement (BC-600, Saint-Gobain) and afterwards introduced to the light guide at both ends of the plate. The soundness of all WLS fibers were tested by measuring light yield at one end of the fibers while a LED light (430 nm) illuminated their other end. After waiting for 48 hours for the optical cement to be hardened enough, we placed the scintillator in < 1 Pa vacuum for more than 48 hours to extract outgas from the glued scintillators. The scintillators were wrapped by a 12- μm -thick aluminized mylar, and the MPPCs were respectively attached to the light guide and were fixed by aluminum plates.

Four MPPCs are attached to each side of the DCV scintillator and operated at a common high voltage. A MPPC gain was measured using a single photoelectron spectrum to group MPPCs with similar gains.

The light yield of the assembled scintillator was measured by using cosmic-rays triggered at eight different positions of the plates. As shown in Figure 4, the average number of photoelectrons for 0.8 MeV energy deposited by cosmic-rays hitting the center of the scintillator was 60.2 for the DCV1 and 58.6 for the DCV2. The light attenuation lengths were (2469 ± 165.1) mm for the DCV1 and (2566 ± 166.0) mm for the DCV2, respectively.

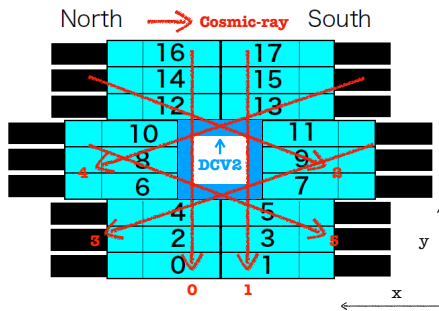


Figure 5. Tracks of the cosmic-rays identified by the CC05 for the DCV2 calibration.

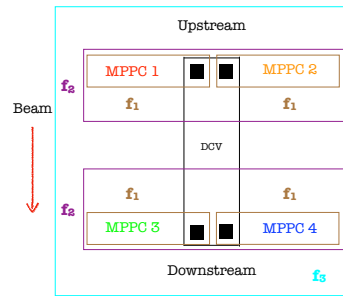


Figure 6. Three different gain factors for the DCV energy calibration with 4 MPPCs.

4. Energy Calibration

After the installation of the DCV, we took cosmic-ray data for its energy calibration. We used two detectors made of CsI crystals and surrounding the DCV (i.e. the CC04 for the DCV1 and the CC05 for the DCV2) as the trigger counter. We can select a track of the cosmic-ray by using the detectors as shown in Figure 5, and estimate the amount of energy deposits by the cosmic-ray in the DCV. Since the scintillation light was shared by 4 MPPCs, we needed to extract gain factors for them to produce an energy deposit after summing up. As the first step, we selected the tracks passing through only half parts of the DCV in which a clear peak in the ADC distribution can be obtained at single MPPC. For example, track 1 was used to get the ADC distribution for MPPCs placed at the south parts of the top and bottom plates. After fitting the Landau distribution convoluted with Gaussian to the obtained ADC distributions of each MPPC, we evaluated the gain factor f_1 from the MPV value for them individually. Secondly, we corrected for the effect of shower sharing (f_2) by summing up calibrated ADC values with the f_1 for two MPPCs at both ends individually and fitted again the same function. Finally, we summed 4 calibrated ADC values, we applied the two factors (f_1 and f_2) at the same time and fitted again to obtain the gain factor f_3 . Figure 6 shows the regions in which each

factor was calculated.

During the beam time from February to April in 2019, we collected the cosmic-ray data at the accelerator maintenance day once in a week. Figure 7 shows gain factors for whole MPPCs and variation according to time of data taking. The gain factors tend to increase over time which implies that the gains of MPPCs decrease. A detailed study on the variation is undergoing.

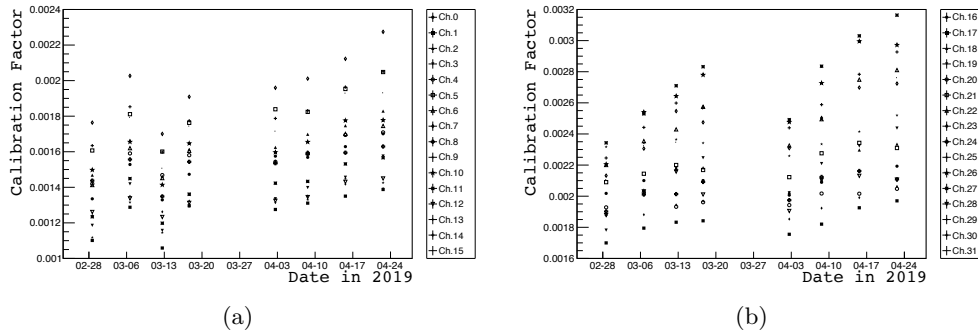


Figure 7. Calibration Factor over time for DCV1 (a) and DCV2 (b).

5. Summary

We fabricated and installed a new charged particle detector DCV for further rejection of the background events from the $K_L \rightarrow \pi^+\pi^-\pi^0$ decay. Based on the cosmic-ray test performed during its fabrication, the light yield is 60 photoelectrons for 0.8 MeV energy deposit at the center of the DCV. We established a method for its calibration by using cosmic-ray identified by detectors surrounding the DCV. Long-term stability of the DCV performance is now under study.

Acknowledgements

This work is supported by the National Research Foundation of Korea-2017R1A2B4006359, and the JSPS KAKENHI Grant No. JP23224007 and No.17K05480.

Reference

- [1] Ahn J K *et al.* 2019 *Phys. Rev. Lett.* **122** 021802